

Department of Chemistry

Facilities at Chemistry Research Centre



[MUFFLE FURNACE 900 °C]

[HIGH TEMPERATURE FURNACE - 1300 °C]

TECHNICO

TECHNICO



THERMOSTAT




U.V.VISIBLE SPECTROPHOTOMETER -- LABMAN



**SCHIMADZU HIGH
PRECISION BALANCE**



K-ROY SINGLE PAN BALANCE

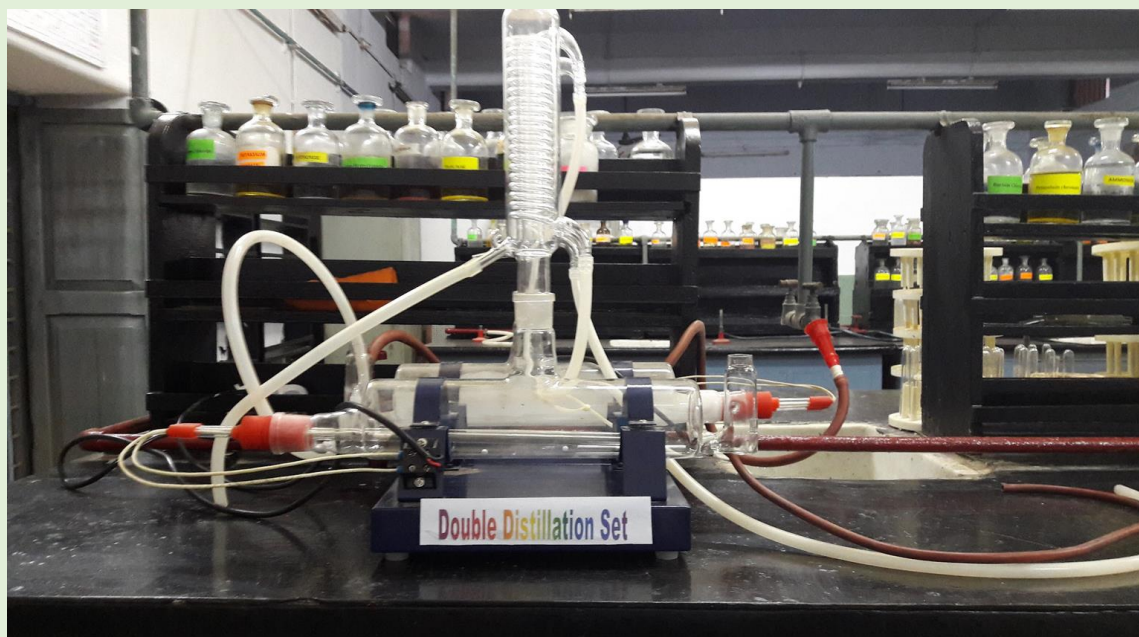

DOUBLE DISTILLATION SET



HOT PLATE



WATER BATH



DE-IONIZER

INSTRUMENTATION AT UG CHEMISTRY LABS



Digital Conductivity Meter
Company : Systronics



Ion Exchanger
Company :
Wation 050200



Digital Potentio Meter
Company : Systronics



Hot Air Oven
Company :
Kemi




Digital Colori Meter 115
Company : Systronics



Muffle Furnace
Company :
Kemi




Magnetic Sturrer with Hot Plate
Company : Infra



Distilation Apparatus
Company :
Borocil Glass Wear



Melting Point Apparatus
Company : Edison



Fractional Distilation Apparatus
Company :
Borocil Glass Wear



Digital Electronic Balance
Company : Infra



DIGITAL ELECTRONIC BALANCE



MAGNETIC STIRRER



MELTING POINT APPARATUS




HEATING MANTLE



CENTRIFUGE MACHINE



DESICCATOR

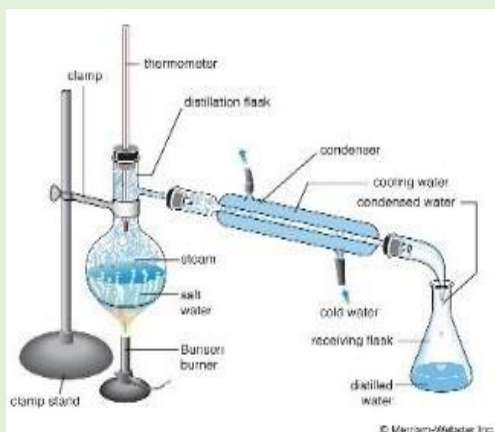

SIMPLE DISTILLATION APPARATUS



DIGITAL PH METER



DIGITAL POTENTIOMETER



DIGITAL CONDUCTIVITY METER



DIGITAL COLORIMETER





DIGITAL COLORIMETER



DIGITAL ELECTRONIC BALANCE

CHROMATOGRAPHY TECHNIQUES

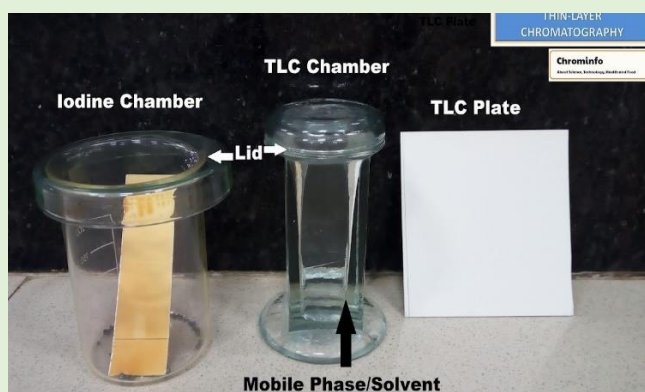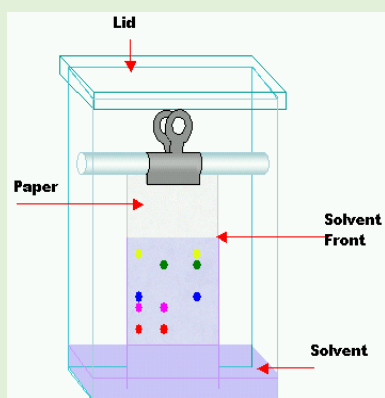

THIN LAYER CHROMATOGRAPHY



COLUMN CHROMATOGRAPHY

SOIL TESTING KIT



DIGITAL P^H METER